

1/5

Fig. 1


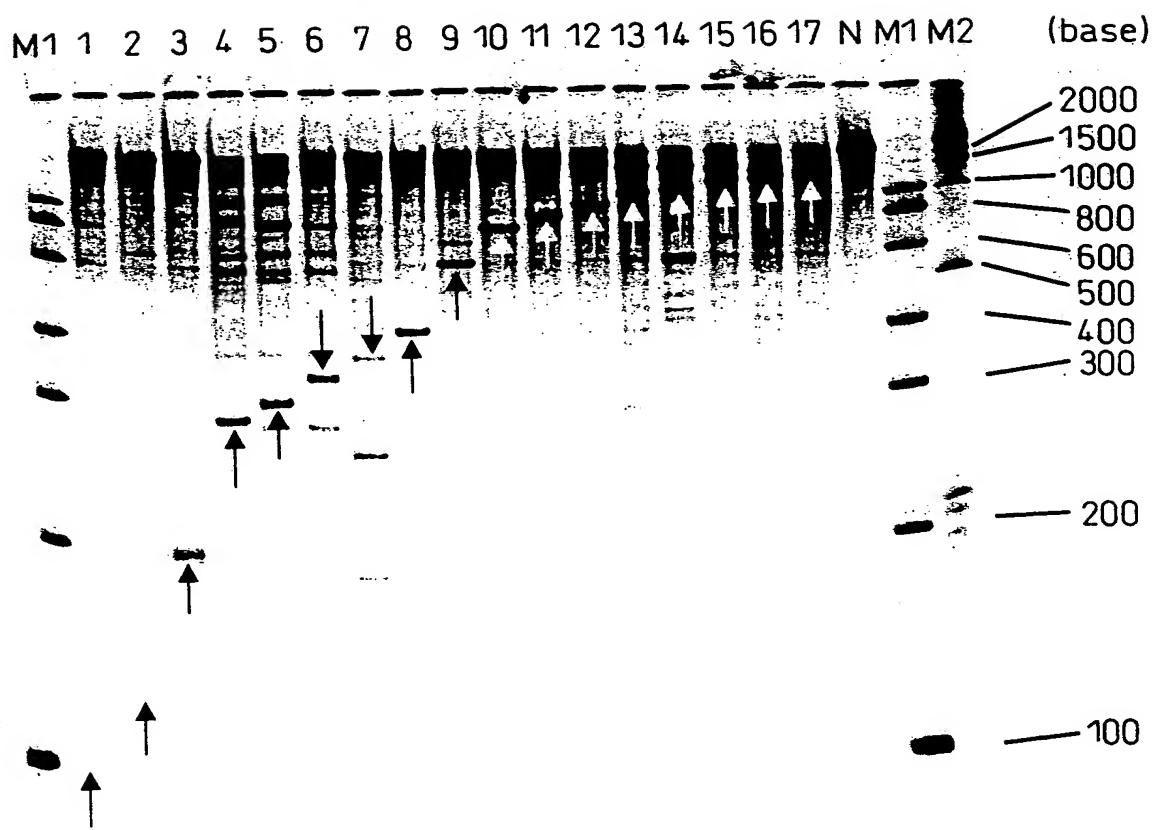


Fig. 2

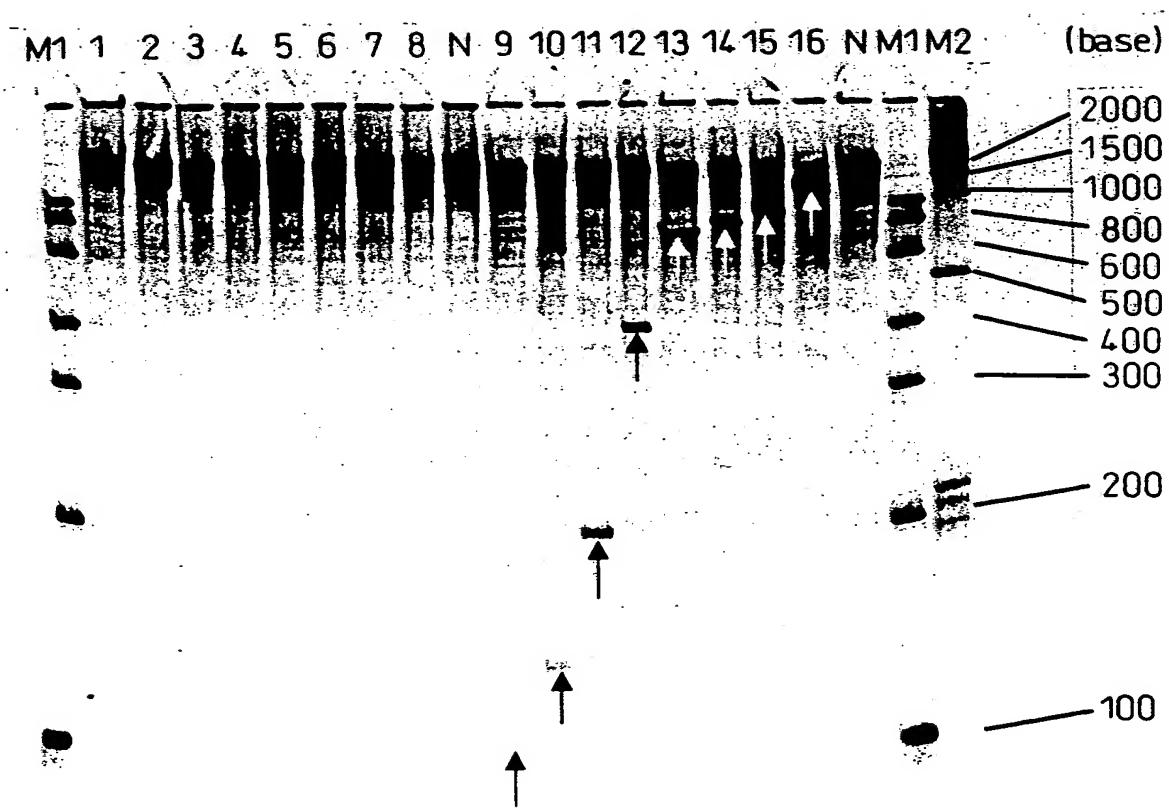

~~3/5~~

Fig.3



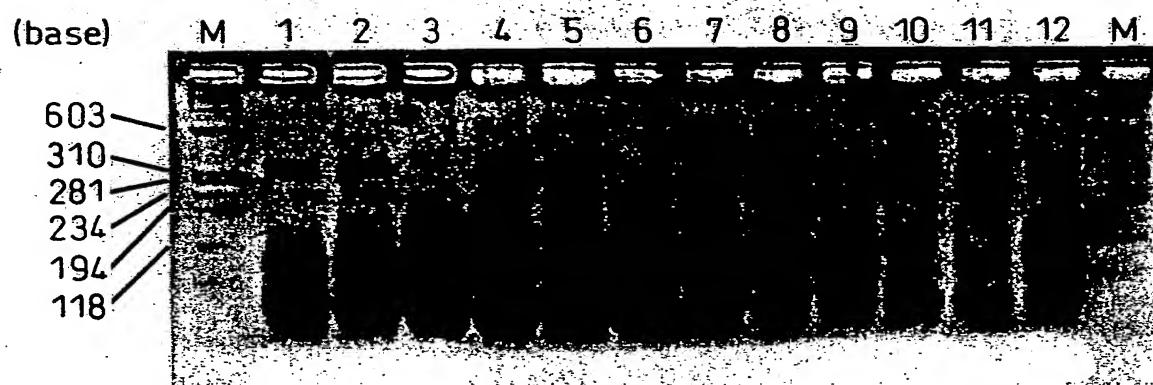


Fig.4

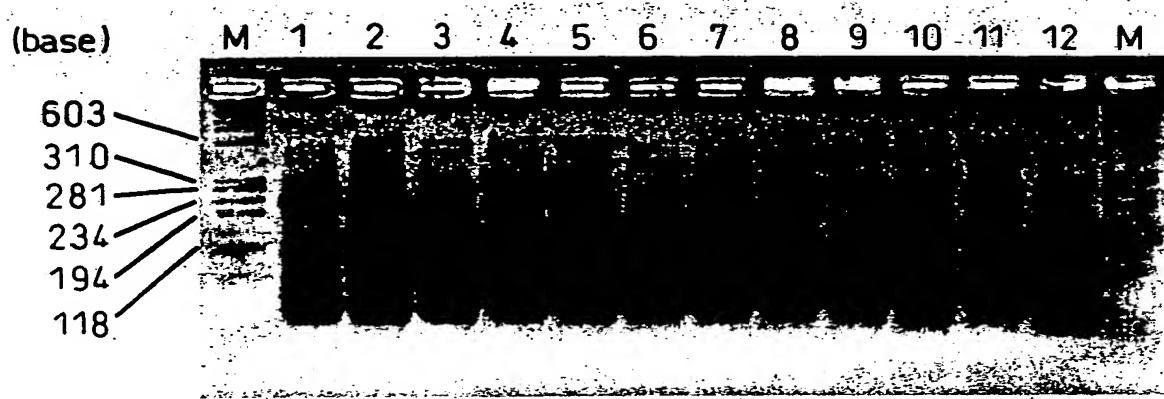

~~4~~/5

Fig.5

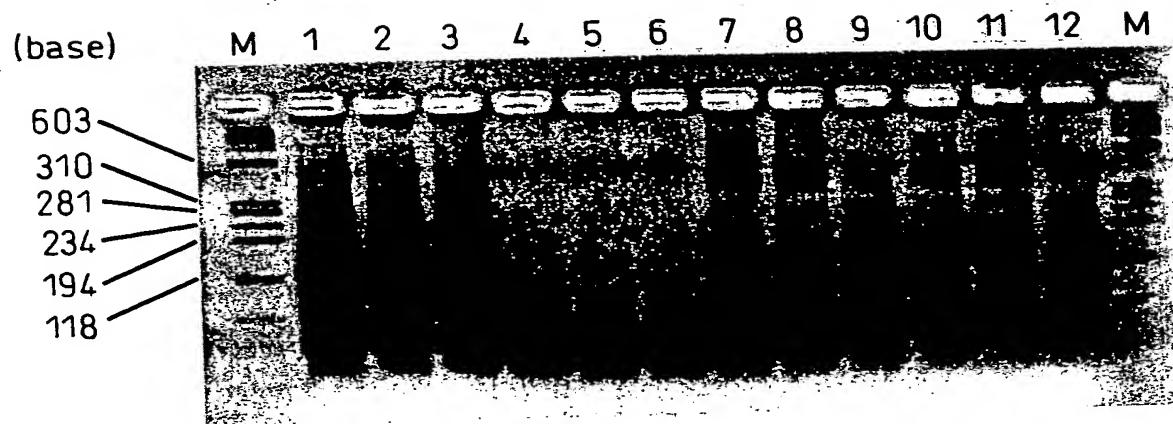


5/5

Fig. 6

(A)

FLUORESCENCE PROFILE

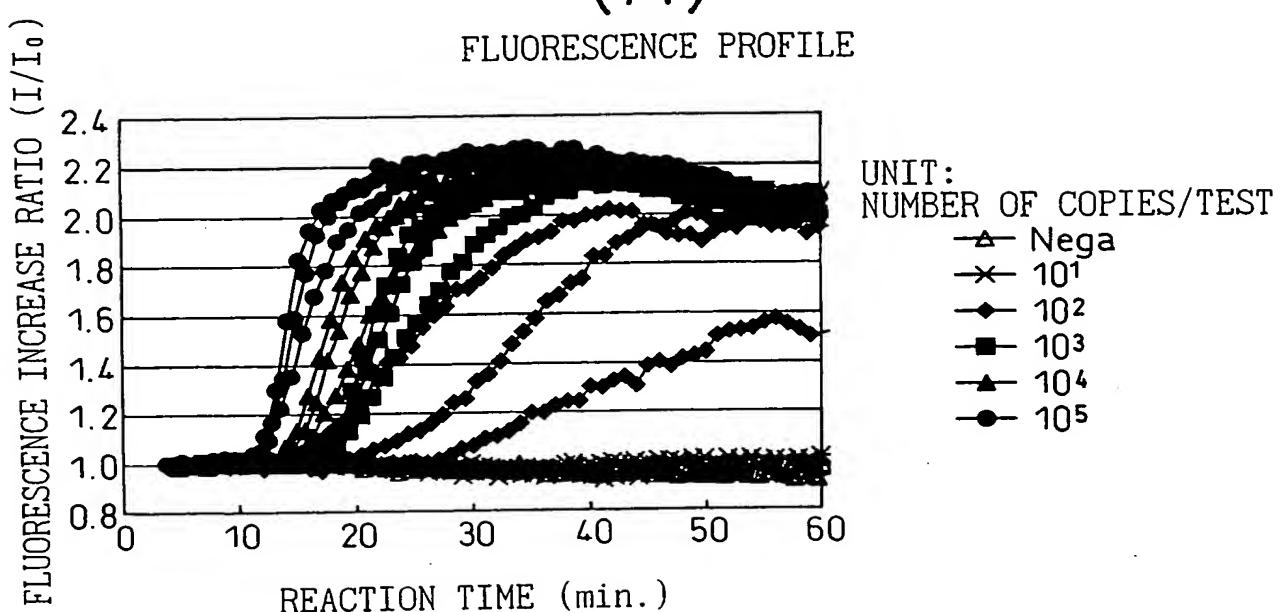

(B)

CALIBRATION CURVE

